

# Point Pivot

*Instructions for Use*



This document provides information for the prosthetists who will be installing the Point Pivot.

Refer to [www.pointdesignsllc.com/resources](http://www.pointdesignsllc.com/resources) to ensure you have the latest copy of this document.



point designs  
1216 Commerce Ct., Ste 3  
Lafayette, CO 80026  
USA  
(720) 600-4753  
[www.pointdesignsllc.com](http://www.pointdesignsllc.com)  
[info@pointdesignsllc.com](mailto:info@pointdesignsllc.com)

**Rx ONLY**

**Caution:** Federal law restricts this device to sale by or on the order of a prosthetist.



*This symbol is used throughout the guide to indicate important cautionary information. Text following this symbol should be read carefully.*

# Point Pivot

*INSTRUCTIONS FOR USE*

*V1.0*

*AUGUST 16, 2023*

**Thank you for choosing the Point Pivot and providing your client with an effective and robust dynamic mounting solution.**

Whether you are retrofitting the Point Pivot into an existing prosthetic socket or you are building a new prosthesis from the ground up, this guide will familiarize you with the functionality and installation of the Point Pivot.

The installation of any Point Pivot should be performed exclusively by a licensed prosthetist or technician. Point Pivot is intended to be operated by a prosthesis user following installation and setup. Any unauthorized handling or installation of a Point Pivot could void its warranty.

Any questions? We are always happy to help.  
Call us or send us an e-mail.

**(720) 600-4753**

**support@pointdesignsllc.com**

# Point Pivot

## Intended Use

The Point Pivot is a prosthetic device that is a reusable, non-sterile, non-active, and non-invasive medical device. It is used for long term compensation of a disability. It is used exclusively for external prosthetic fittings of the upper limbs. It is intended to provide rotation of the thumb flexion-extension plane at the metacarpal phalangeal joint in order to generate stable hand grasps. The Point Pivot is intended to be fit on people with amputations of the thumb slightly proximal of the metacarpal phalangeal (MCP) joint. The patient population is not specific, and it is used by lay persons and health professionals in clinical, home, working and/or industrial environment. The Point Pivot system is used in combination with the Point Thumb and a prosthetic socket.

## Indications

Users of the Point Pivot system will achieve the best clinical outcome if they have amputation of the thumb slightly proximal of the MCP joint (through the MCP joint or slightly distal of the MCP joint is also acceptable).

## Intended Patient Population

The Point Pivot is intended to be fit on people with amputations of the thumb slightly proximal of the MCP joint.. The patient population is not specific, and it is used by lay persons and health professionals in clinical, home, working and/or industrial environment. The Point Pivot system is used in combination with the Point Thumb and a prosthetic socket.

## Intended Users

The Point Pivot is to be installed into a prosthetic socket by a trained prosthetist and used by partial hand amputees. The Point Pivot is compatible with most prosthetic sockets and is installed into the prosthetic socket by a trained prosthetist or technician.


## Contraindications

None known.

# Table of Contents

Introduction to the Point Pivot .....	6
Component Description .....	7
<i>Point Pivot unit</i> .....	7
<i>Lamination spacer</i> .....	7
<i>Mounting screws</i> .....	7
<i>Mounting bracket</i> .....	8
Specifications .....	9
Installation .....	10
<i>Included in the package</i> .....	10
<i>What you will need</i> .....	10
<i>Positioning</i> .....	11
<i>Lamination</i> .....	13
<i>Prefitting Function Checklist</i> .....	14
Using the Point Pivot .....	15
<i>Before you begin</i> .....	15
<i>Rotation</i> .....	16
Troubleshooting .....	17
Maintaining The Point Pivot .....	18
<i>Preventative Inspection</i> .....	18
<i>Maintenance</i> .....	18
<i>Disposal</i> .....	18
<i>Repairs, Returns and Warranty</i> .....	18
Safety and Warnings .....	19
Annex I .....	24

# Introduction to the Point Pivot

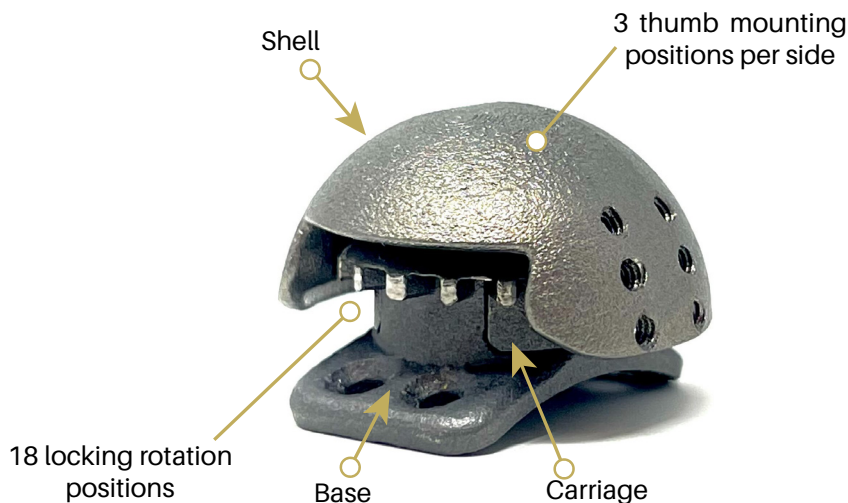

The **Point Pivot** is a dynamic mounting system that provides an additional degree of freedom to the Point Thumb. As a replacement to the standard mounting for the Point Thumb, the **Point Pivot** enables 18 positions of rotation of the plane that the thumb flexion-extension plane, allowing for a greater number of achievable hand grasps. The **Point Pivot** is made from titanium for ample strength.

A Point Thumb attached to a **Point Pivot** can be rotated by applying a downward force and turning it clockwise or counterclockwise.

A single **Point Pivot** can be integrated into a prosthetic socket using the mounting kit.

The Point Pivot comes in two configurations: *Compact* and *Extended*. By default the Point Pivot is provided in the Compact configuration. The Extended configuration can be provided upon request. The Extended configuration is intended only for retrofitting the Point Pivot onto existing sockets.



Compact Configuration



Extended Configuration

# Component description

## THE POINT PIVOT



Point Pivot  
*Compact OR Extended*




Torx Tool



The Point Pivot comes assembled as one unit and is comprised of a curved base, carriage, shell, and an internal spring. The base has 4 mounting holes for attaching to a prosthetic socket.

## LAMINATION SPACER

The lamination spacer helps maintain mounting hole alignment and structural rigidity during the lamination process and prevents resin from seeping into the mounting area or mounting holes. Only the **Compact** configuration comes with a lamination spacer

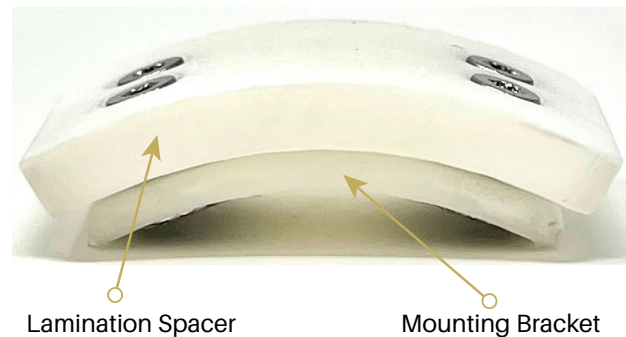

## MOUNTING SCREWS


Two different sets of Torx mounting screws are included with the Point Pivot. Eight (8) M2 x 5mm screws are for attaching the lamination spacer to the bracket during the lamination process and for mounting the base of the Point Pivot to the bracket. Eight (8) M2 x 4mm screws are for attaching the Point Thumb to the Point Pivot shell.



# Component description

## MOUNTING BRACKET

M2 x 5mm Mounting  
Screws

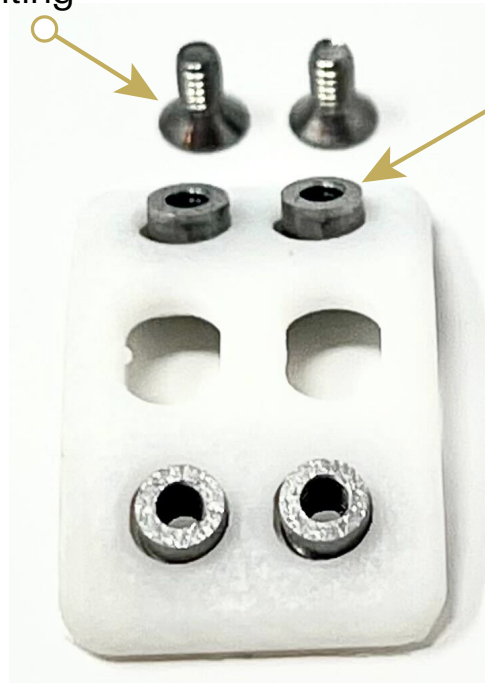

Mounting Area

The mounting bracket is comprised of a mounting area and slots through which to weave carbon fiber to create a robust lamination. Only the *Compact* configuration comes with a mounting bracket.



# Specifications

<b>Material</b>	<i>Titanium</i>
<b>Rated load</b>	<i>667 N (150 lbf)</i>
<b>Rated torque</b>	<i>8 Nm (5.9 ft-lbf)</i>

# Installation

## INCLUDED IN THE PACKAGE

### Compact Configuration

- One (1) Point Pivot - Compact
- One (1) Point Thumb (*ordered separately*)
- One (1) Mounting Kit, consisting of:
  - One (1) lamination spacer
  - One (1) mounting bracket
  - Eight (8) M2 x 4mm mounting screws
  - Eight (8) M2 x 4mm mounting screws
  - Torx tool size T6

### Extended Configuration

- One (1) Point Pivot - Extended
- One (1) Point Thumb (*ordered separately*)
- One (1) Mounting Kit, consisting of:
  - Eight (8) M2 x 4mm mounting screws
  - Eight (8) M2 x 4mm mounting screws
  - Torx tool size T6

## WHAT YOU WILL NEED

- Prefabricated patient socket (e.g., carbon fiber & silicone)
- Lamination supplies (e.g., prepreg carbon fiber, adhesive, silicone, etc.)
- Lamination tools (Dremel, files, PVA bag, etc.)
- Blue thread locker (Loctite Blue 242 or similar)

## BEFORE YOU BEGIN

If using the **Compact** configuration, follow all of the steps in the Installation section. If using the **Extended** configuration, only follow step 1 in the Positioning sub-section and then step 19 in the Lamination sub-section as you will be simply mounting the **Point Pivot** and **Point Thumb** to an existing socket.

# Installation


## POSITIONING

1. Mount the Point Thumb to the shell of the Point Pivot using the M2 x 4mm mounting screws and T6 Torx tool. Apply threadlocker. Note that you can mount the Point Thumb in 6 possible positions (3 in each direction) depending on the desired alignment.



2. Attach the mounting bracket to the Point Pivot using the M2 x 5 mm mounting screws and T6 Torx tool.

Point Pivot

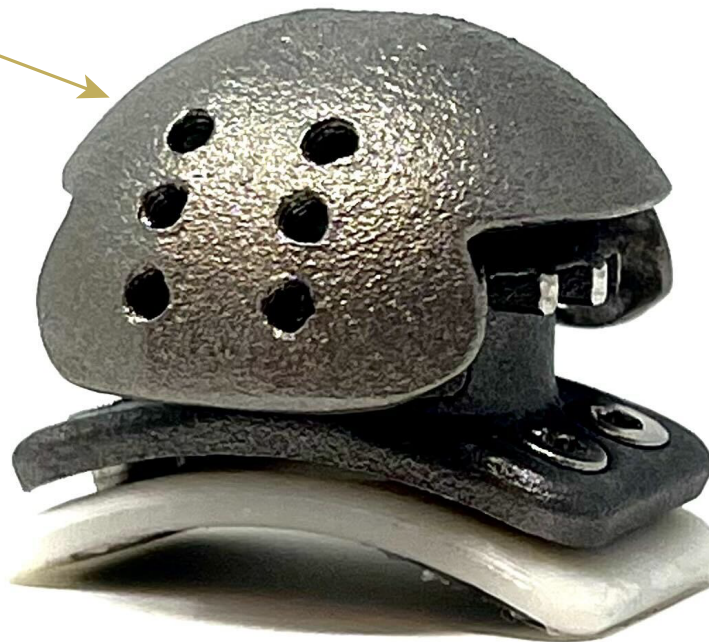

Mounting Bracket



# Installation

## POSITIONING

3. With the mounting bracket attached, align the **Point Pivot** on the carbon shell as desired.
4. Use your preferred adhesive to tack the mounting bracket into position, then remove the **Point Pivot** using the Torx tool.
5. Apply additional adhesive to create a secure bond to the mounting bracket.
6. Remount the **Point Pivot** using the supplied mounting hardware and Torx tool. Inspect the clearance around the **Point Pivot** mounts, considering there will be some layers of prepreg carbon fiber added later.
7. Check that the **Point Pivot** shell can depress fully and rotate into each rotational locking position. Also check that the Point Thumb can reach full flexion. If these functions cannot be achieved, then adjust the position of the Point Pivot on the carbon shell. Remove the **Point Pivot**.

# Installation

## LAMINATION

1. Mount the lamination spacer using the M2 x 5mm mounting screws and Torx tool.
2. Check the clearance between the lamination spacer and the adhesive.
3. Shape adhesive with dremel (or similar) as needed.
4. Remove the lamination spacer.
5. Reinforce the mounting bracket by weaving two strips of carbon fiber through the central slots of the mounting bracket. Lay an additional strip perpendicular to those two strips and running between the raised threaded bosses.
6. Pack carbon prepreg under/around the mounting brackets to fill any voids.
7. Add carbon prepreg to fill the area over the brackets up to the height of the thread mounts.
8. Add carbon prepreg over the entire model excluding the threaded mounting faces.
9. Apply a very thin layer of non-curing silicone to the bottom part of the lamination spacer so it will form to the prepreg and apply pressure.
10. Fill the threaded mounting holes with silicone grease to ease later removal of screws by preventing prepreg epoxy from flowing into threads.
11. Reapply the lamination spacer using supplied mounting hardware and the Torx tool.
12. Remove excess silicone that is pressed out during reapplication of the lamination spacer.
13. Apply more silicone putty to blend the bottom part of the lamination spacer to the model.
14. Fill over mounting screw with silicone.
15. Apply PVA bag under the prepreg shell.
16. Apply second PVA bag over the entire model.
17. Apply vacuum.
18. After curing is complete and the model has cooled, clean the prepreg and remove both parts of the lamination spacer.
19. Mount the **Point Pivot** using the M2 x 5mm mounting screws and Torx tool. Apply threadlocker to mounting hardware. Inspect the **Point Pivot** for proper function.

# Installation

## *PREFITTING FUNCTION CHECKLIST*

The prosthetist should ensure that all the following functions are checked prior to fitting the user with the prosthesis.

If any of the functions are not working properly, please either review the installation instructions and/or contact **support@pointdesignsllc.com**

- Ensure the shell can be depressed.
- Ensure the shell can be rotated and locked into all 18 locking positions.
- Ensure that the Point Thumb can reach full flexion and spring back to full extension

# Using The Point Pivot

## ROTATION



Rotate Clockwise

Push Digit  
Down



Rotate Counterclockwise

1. Apply a downward force and rotate the attached digit into one of eighteen locking positions. When the digit is released, the device will automatically lock into place.

# Troubleshooting

*In case of a problem, this section is intended to help you troubleshoot the operation of the Point Pivot.*

*We have included a few possible issues with solutions below.  
If your issue is not addressed, email us for support at [support@pointdesignsllc.com](mailto:support@pointdesignsllc.com).*

## **Point Pivot shell does not depress to allow for rotation**

There is likely debris obstructing the rotation mechanism. Clean the inside of the carriage with compressed air to remove the debris.

## **Point Pivot is loose or came off mounting bracket**

Make sure thread locker has been applied to Torx screws, and then tighten them. If Torx screws are unable to be tightened, contact us for additional support.

## **Point Pivot is corroded.**

Contact us for support.



Users and/or patients should report any serious incident that has occurred in relation to the device to:

- Point Designs at [support@pointdesignsllc.com](mailto:support@pointdesignsllc.com)
- FDA via MAUDE (for cases in US)
- The competent authority of the Member States in which they are established in EU/EEA (for cases in the EU/EEA)



# Maintaining Point Pivot

## PREVENTATIVE INSPECTION

All **Point Pivot** systems undergo extensive quality assurance inspections prior to shipping. Regularly inspect **Point Pivot** for dirt/grime in the rotation teeth. Clean **Point Pivot** (see MAINTENANCE section below) if decreased performance occurs.

## MAINTENANCE

The **Point Pivot** can be cleaned with a cleaning solution such as soap + water or detergent + water. Dry the device with a clean towel or compressed air. Be sure to dry the device completely after getting wet, especially when the liquid is likely to accelerate corrosion (e.g., salt, water, sweat, etc.).

Lubrication (e.g., WD-40, graphite, etc.) may be applied to the joints and track after cleaning if increased resistance occurs.

For any abnormal issues, discontinue use and contact Point Designs for support.

## DISPOSAL



A **Point Pivot** should not be thrown away with common household waste. Dispose of the **Point Pivot** by either returning the unit to Point Designs or taking the unit to your nearest metal recycling center.

## REPAIRS, RETURNS + WARRANTY

Please contact Point Designs at [support@pointdesignsllc.com](mailto:support@pointdesignsllc.com) regarding repairs and returns. The **Point Pivot** comes with a 1-year manufacturer's defect warranty.

Details of the warranty are in separate documentation available at [www.pointdesignsllc.com/resources](http://www.pointdesignsllc.com/resources).

# Safety and Warnings



**WARNING:** The Point Pivot is not designed to operate continuously in wet environments. A Point Pivot may get wet occasionally, but the user should be advised to thoroughly dry the Point Pivot after exposure to any liquid. Prolonged exposure to liquid may cause corrosion.



**WARNING:** The Point Pivot is electrically conductive and thus presents a potential electric shock hazard if it contacts a voltage difference and the user's (or someone else's) skin simultaneously. The Point Pivot should not be used around high voltage/current.



**WARNING:** The Point Pivot is thermally conductive and thus presents a potential burn hazard if it contacts a heat source and then the user's (or someone else's) skin subsequently. The Point Pivot should be kept away from hot objects. If a Point Pivot becomes hot, it should be allowed to cool before skin contact.



**WARNING:** The Point Pivot contains ferrous material, and can therefore interact with magnetic fields. Care should be taken when using a Point Pivot around magnets to avoid accidental attraction. For example, *keep away from MRI machines.*



**WARNING:** The Point Pivot contains moving parts (e.g., springs, ratcheting mechanisms, etc.), and thus presents a minor pinching hazard. The user should take care to keep loose skin, clothing, etc. from the moving parts of the Point Pivot.



**WARNING:** The Point Pivot contains internal springs under tension.



**WARNING:** Any unauthorized modification to a Point Pivot System can pose a safety risk to the user and will void the warranty. Changes or modifications not expressly approved by Point Designs could void the user's authority to operate the equipment.



**WARNING:** The end user is the intended operator of the device and is responsible for its use.



**WARNING:** The Point Pivot does not provide sensation; heat and moisture cannot be felt.



**WARNING:** Do not disassemble componentry or modify in any way.



**WARNING:** Do not service or perform maintenance when in use.



**WARNING:** Do not use with machinery with moving parts that may cause personal injury or damage.



**WARNING:** Do not use for extreme activities that may cause injury to a natural hand.



**WARNING:** Do not expose to excessive or high forces, particularly on the fingertips and on the side of the digits.



**WARNING:** Do not expose to excessive moisture, liquids, dust, high temperatures, or shock.



**WARNING:** Do not use in hazardous environments.



**WARNING:** Do not expose to high temperatures.



**WARNING:** Do not expose to flames.



**WARNING:** Do not use in or expose to explosive atmospheres.

\* Warnings covered in this section are residual risks associated with use of the Point Pivot



**PRECAUTION:** Users must comply with local regulations on the operation of automobiles, aircraft, sailing vessels of any kind and any other motorized vehicle or device. It is entirely the user's responsibility to seek confirmation that they are physically and legally able to drive using the **Point Pivot** and to the fullest extent permitted by law.












**PRECAUTION:** Only use with approved Point Designs accessories and tooling.



**PRECAUTION:** Maintenance, repairs, and upgrades may only be performed by qualified Point Designs technicians and technical partners. Point Designs will provide, upon request, information to assist service personnel in repair of a device.

# Annex I

## DESCRIPTION OF SYMBOLS FROM PRODUCT LABEL

Symbol	Description
	CATALOG/PART NUMBER
	CAUTION
	DATE OF MANUFACTURE
	EUROPEAN AUTHORIZED REPRESENTATIVE
	REFER TO INSTRUCTIONS FOR USE
	LOT NUMBER/BATCH CODE
	MANUFACTURER
	MEDICAL DEVICE
	SERIAL NUMBER

# NOTES



# NOTES



point designs

[www.pointdesignsllc.com](http://www.pointdesignsllc.com)

[info@pointdesignsllc.com](mailto:info@pointdesignsllc.com)

(720) 600-4753